

Original Article

Effects of removing adhesive from tooth surfaces by Er:YAG laser and a composite bur on enamel surface roughness and pulp chamber temperature

Sogra Yassaei¹, Hossein Aghili¹, Neda Joshan¹

¹Department of Orthodontics, School of Dentistry, Shahid Sadoughi University of Medical Sciences, Yazd, Iran

ABSTRACT

Background: At the end of fixed orthodontic treatment, the remnant of adhesive should be eliminated from the tooth surface. The purpose of this study was to compare the effect of three methods of removing adhesive on enamel surface roughness, dental pulp temperature, and also on the time spent.

Materials and Methods: The brackets on 90 extracted teeth were debonded using bracket removal pliers. A thermocouple sensor was fitted on the buccal wall of the pulp chamber through access cavity to measure thermal changes during adhesive removal. The residue of adhesive was eliminated from enamel surface of teeth by either tungsten carbide bur, erbium-doped yttrium aluminum garnet laser, or fiber reinforced composite bur. Scanning electron micrographs images were taken to assess the roughness of enamel surface. The time spent for adhesive removal was recorded as well. Chi-square test was used to evaluate the remnants of adhesive and enamel surface roughness; *t*-test and also repeated measurement analysis of variance were applied at $P < 0.05$ to compare the thermal changes of the pulp chamber and time spent between the methods of surface treatment.

Results: The results of surface roughness were significantly different ($P < 0.001$). The pulp temperature changed significantly ($P < 0.001$). Tungsten carbide bur increased the temperature by 5.5°C significantly slower than reinforced composite bur ($P = 0.004$), however removed the adhesive residue faster than two other methods although not significantly ($P = 0.069$).

Conclusion: Within the limitations of this study, fiber reinforced composite bur created the smoothest enamel surface while Er:YAG laser the roughest. Tungsten carbide and composite burs generated more heat compared to Er:YAG laser. In addition, tungsten carbide bur was the fastest and Er:YAG laser the slowest devices to remove adhesive residue.

Key Words: Adhesive removal, composite bur, laser, pulp temperature, surface roughness

Received: December 2013
Accepted: March 2015

Address for correspondence:

Dr. Neda Joshan,
Department of
Orthodontics, School of
Dentistry, Shahid Sadoughi
University of Medical
Sciences, Dahe Fajr Blvd,
Imam Ave.,
PO Box 89195/165,
Yazd, Iran.
E-mail: neda.joshan@
gmail.com

INTRODUCTION

Following completion of fixed orthodontic treatments and debonding of the brackets, the remnants of adhesive should be eliminated in a manner that tooth

enamel remains as intact as possible. Change in the superficial layer of enamel, with the most content of minerals and fluoride, is orthodontists' concern because following the loss of enamel surface, and exposure of enamel prisms to the mouth environment and organic acids in dental plaque, the susceptibility to decalcification increases.^[1]

Remnants of adhesive on enamel surface can be eliminated through different methods and instruments including: Finishing carbide bur,^[2] bioactive glass air abrasion,^[3] tungsten carbide bur in low or high speed hand pieces,^[4] aluminum oxide air abrasion.^[5,6] Rotary instrument is the contemporary technique to remove

Access this article online



Website: <http://drj.mui.ac.ir/index.php/drj>
<http://www.ncbi.nlm.nih.gov/pmc/journals/1480/>

adhesive.^[2] Mechanical elimination of adhesives, which are tooth colored materials, is associated with some degree of damages to enamel surface.^[7] Studies show that conventional methods of adhesive removal including: Ultrasonic and hand scalers, and low speed handpiece with abrasive create visible surface roughness, 10-20 μm deep gouges, and loss of 100 μm thickness of enamel.^[8] Therefore, any improvement in the technique of adhesive removal is welcomed by orthodontists. In addition, to conventional techniques, fiber reinforced composite burs and different kinds of laser such as free running erbium-doped yttrium aluminum garnet (Er:YAG),^[9,10] neodymium-doped yttrium aluminum garnet,^[11,12] XeCl^[13] and millisecond pulsed CO₂^[14] are investigated. Composite burs were initially designed to remove cement, stain, and colors from the tooth surface and were recommended for adhesive removal following orthodontic debracketing. According to the manufacturer, the fiber sections with abrasive property is the advantage of this bur. These sections of zircon/glass fibers are embedded in a matrix of resin and slowly become disintegrated in contact with a hard surface. Karan *et al.*^[15] used fiber reinforced composite bur to eliminate adhesive residues. They evaluated the surface using atomic force microscopy and concluded that composite bur creates smoother surface compared to tungsten carbide bur. The studies of Almeida *et al.*^[16] and Burkes *et al.*^[17] showed that Er:YAG laser removed greater volume of enamel compared to tungsten carbide bur.

On the other hand, the generated heat during adhesive removal is transferred to the dental pulp and causes histopathological changes that may lead to necrosis through injury to blood vessels.^[18] Zach and Cohen^[19] concluded that raised temperature of the dental pulp tissue by 5.5 ($^{\circ}\text{C}$) causes irreversible inflammation in 40% of cases, and by 11 ($^{\circ}\text{C}$) leads to the dental pulp necrosis. Studies show that Er:YAG laser with water cooling,^[17,18,20] and tungsten carbide bur without water or air cooling^[21] did not significantly raise the temperature of the dental pulp tissue. We could not find any study about the effect of composite burs on temperature.

Time spent for residual adhesive removal is an important factor. David *et al.*^[22] reported a cleanup time of 40 s by tungsten carbide bur in high speed hand piece.

The roughness of enamel surface has been assessed by different devices including: Linear contact measuring

tools, optical three-dimensional scanners, and electron microscopy.^[23] Linear contact measuring tools evaluate a limited area of the enamel surface, but optical three-dimensional scanner considers a large area.^[24] Electron microscopy is a visual analyzer,^[25] which is suitable to evaluate the smoothness of surfaces.^[26]

Considering that no safe method has been suggested to remove residual adhesive,^[26] in this *in vitro* study, the effect of three methods of removing adhesive from enamel surface roughness, dental pulp temperature, and also on the time spent was compared.

MATERIALS AND METHODS

A sample of 90 intact extracted human premolar teeth were randomly placed in three groups of 30, although the estimated sample size of each group, through a pilot study on 10 teeth at 95% coefficient of confidence and the power of 80%, was 21 cases. The teeth were kept in distilled water^[25] for not more than 1 month. The water was renewed every week.^[26] Following cleaning the buccal surface of teeth with fluoride free pumice paste and rubber cup in low speed handpiece, the teeth were rinsed with water and dried by air stream. Then, the surfaces were etched by phosphoric acid gel 37% (Etching agent, Resilient ortho technology, Florida, USA) for 30 s, rinsed for 15 s, and dried to appear a matt and chalky surface.^[26] A thin layer of adhesive (Resilient ortho technology, Florida, USA) was applied by a micro brush on the etched surface. A standard stainless steel edgewise premolar bracket (GAC, Central Islip, New York, NY, USA) was attached to enamel surface with composite (Resilience Ortho technology, Florida, USA), then all four edges were light cured (Top light, Taiwan) for 40 s after removing the excess composite. The samples were incubated in water for 24 h at 37 ($^{\circ}\text{C}$)^[21] before debracketing by bracket removal pliers (Ormco, CA, USA). An access to the pulp chamber was prepared in lingual surface. The teeth were divided randomly into three equal groups. Teeth surfaces were explored by microscope at $\times 35$ magnification to assess the adhesive residue. According to adhesive remnant index (ARI), described by Artun and Bergland,^[27] teeth were categorized in 4 grades: 0 = no adhesive, 1 = Less than 50% of adhesive, 2 = More than 50% of adhesive and 3 = All the adhesive remains on the tooth surface. Since no difference was found between three groups [Table 1], we tried to remove the remnant of adhesive by either eight bladed tungsten carbide

Table 1: Distribution of ARI

Groups ARI score*	Composite bur	Tungsten carbide bur	Er:YAG
0	0	0	0
1	3	6	5
2	26	23	23
3	1	1	2

$\chi^2 = 1.75$; $P = 0.78$; Values are presented as number only. $P < 0.05$ indicates a significant result after Chi-square test; Er:YAG: Erbium-doped yttrium aluminum garnet; ARI: Adhesive remnant index, *ARI scores-0: No composite remains on tooth surface; 1: Less than 50% of the composite remains on tooth surface; 2: More than 50% of the composite remains on tooth surface; 3: All of the composite remains on tooth surface.

bur (Geber, Brasseler, Komet-Lemgo, Germany) in low speed handpiece; Er:YAG laser at 2.94 μm , 20 Hz, 125 mJ, 2.5 W and at the distance of 5 mm; and zircon-rich glass fiber reinforced composite bur (Stainbuster Abrasive Technology Inc., Lewis Center, OH, USA) in low speed hand piece. A thermocouple sensor, connected to a microcontroller, was installed on the buccal wall of the pulp chamber through the access hole. The micro controller was recording time and temperature during the process of removing the adhesive.

Enamel surface roughness was evaluated using scanning electron micrographs (SEM) at $\times 100$ magnification. The texture of the surface was interpreted by enamel damage index, introduced by Howell and Weekes.^[28] In this index: Grade 0 is when the surface is smooth without any scratches; Grade 1 is when some scattered scratches are visible; Grade 2 is when the surface is rough with numerous deep scratches and some grooves, and Grade 3 is when deep scratches and wide groves are visible with naked eyes.

Data were analyzed with SPSS 17.0 software package (SPSS Inc., Chicago, Illinois, USA). Chi-square test was used to compare the surface roughness and residual adhesive between groups. *t*-test and also analysis of variance (ANOVA) were used to compare the time spent and thermal changes. The results were evaluated at the $P < 0.05$ significance level, with a 95% confidence interval.

RESULTS

The results of enamel surface roughness, assessed under SEM at $\times 100$ magnification [Figures 1-3], are shown in Table 2. The comparison between groups showed that enamel surface roughness was significantly more in Er:YAG laser group, and

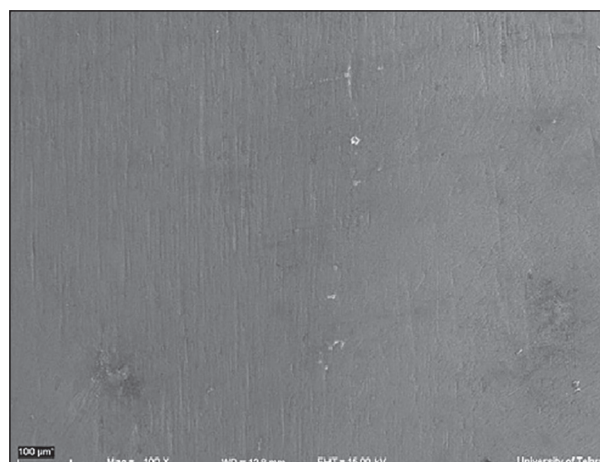


Figure 1: Scanning electron micrograph of a specimen after adhesive removal by composite bur ($\times 100$ magnification).

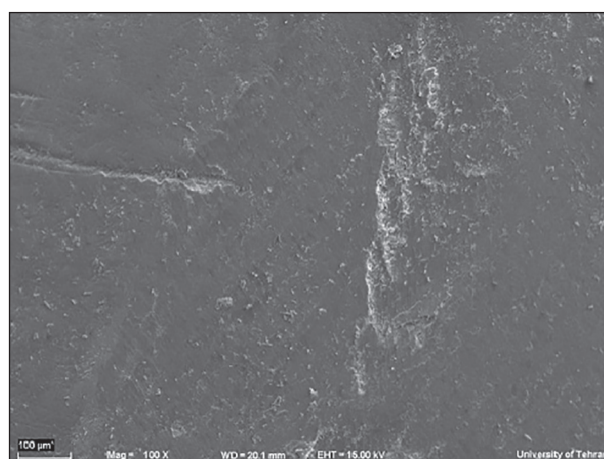


Figure 2: Scanning electron micrograph of a specimen after adhesive removal by tungsten carbide bur ($\times 100$ magnification).

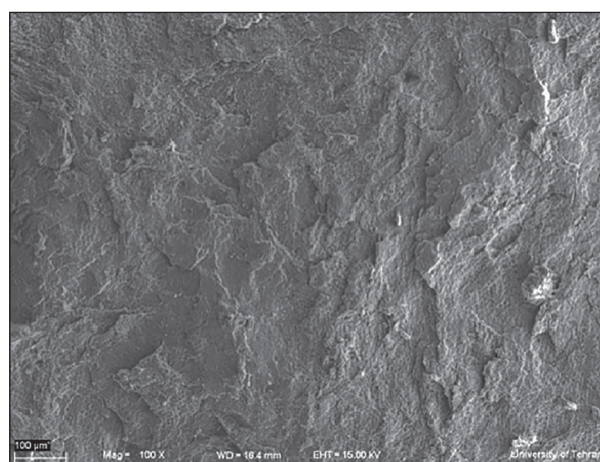


Figure 3: Scanning electron micrograph of a specimen after adhesive removal by erbium-doped yttrium aluminum garnet laser ($\times 100$ magnification).

composite bur created the smoothest surface. Figures 1 through 3 show the post-treatment image of surfaces, which are: Acceptable with fine scattered scratches created by composite bur, with coarse scratches created by tungsten carbide bur, and with wide grooves and numerous coarse scratches created by Er:YAG laser, which was the roughest, respectively.

Comparing the thermal changes in each group showed a significant decrease in Er:YAG laser group, but significant increase in two other groups. The thermal changes in groups are seen in Table 3. ANOVA revealed significant changes in groups.

The time required for increasing the temperature of the pulp chamber by 5.5°C was 56.53 s in tungsten carbide bur, and 37.86 in composite bur groups [Table 4]. In none of the cases of Er:YAG group, the temperature increased by 5.5°C. Four cases of composite bur and four cases of tungsten carbide bur groups did not show an increase in temperature of the pulp chamber by 5.5°C.

Table 5 shows the time spent in groups. The results revealed that although no statistical significant difference was found, but Er:YAG group took the longest time, while the shortest time belonged to tungsten carbide bur group.

DISCUSSION

Regardless of the methods used, some enamel scarring occurs after debracketing and adhesive removal. However, the advantages of bonding orthodontic attachments unquestionably outweigh the disadvantages. Cleaning up of residual bonding resin following debracketing needs to be in a manner that the enamel surface remains intact as much as possible. Hence, the clinician must be aware of the best methods for minimizing enamel damage.

The results of the present study implied that the texture of enamel surfaces, following adhesive removal in the three groups is different. Composite bur created the smoothest, and Er:YAG laser the roughest surfaces, although at the minimum related power setting. Almeida *et al.*^[16] and Burkes *et al.*^[17] showed that Er:YAG laser removed more enamel compared to tungsten carbide bur. In the present study, and the study of Karan *et al.*^[15] tungsten carbide bur created a surface rougher than the composite bur did. This result might be related to disintegration of composite bur in contact with enamel surface while

Table 2: Distribution of enamel damage index* following adhesive removal

Groups	N	Grade 0	Grade 1	Grade 2	Grade 3
Composite bur	30	23	7	0	0
Tungsten carbide bur	30	0	13	15	2
Er:YAG	30	0	0	0	30

Fisher exact test; $P < 0.001$; Values are presented as number only. $P < 0.05$ indicates a significant result after Fisher exact test; *Enamel damage index: Grade 0 is when the surface is smooth without any scratches; Grade 1 is when some scattered scratches are visible; Grade 2 is when the surface is rough with numerous deep scratches and some grooves; Grade 3 is when deep scratches and wide grooves are visible with naked eyes; Er:YAG: Erbium-doped yttrium aluminium garnet.

Table 3: Thermal changes (°C)

Groups	N	Mean ± SD	Minimum	Maximum
Composite bur	30	8.47±3.07	3	13.7
Tungsten carbide bur	30	8.60±3.01	2	14.0
Er:YAG	30	-3.60±1.82	-8	-0.9

ANOVA; $P < 0.001$; $P < 0.05$ indicates a significant result after analysis of variance; Values are presented as number and mean ± SD and minimum and maximum; SD: Standard deviation; Er:YAG: Erbium-doped yttrium aluminum garnet.

Table 4: The time spent (sec) that raised temperature of pulp cavity by 5.5 °C

Groups*	N**	Mean ± SD	Minimum	Maximum
Composite bur	26	37.86±4.2	25	100
Tungsten carbide bur	26	56.53±4.35	25	105

ANOVA; $P = 0.004$; $P < 0.05$ indicates a significant result after analysis of variance; Values are presented as number and mean ± SD and minimum and maximum; *No increase in pulp chamber temperature was seen in Er:YAG group; **Four cases of composite bur and 4 cases of tungsten carbide bur groups did not show increase in temperature of pulp chamber by 5.5 (°C); SD: Standard deviation; Er:YAG: Erbium-doped yttrium aluminum garnet.

Table 5: Time consumed (min) to remove remnants of adhesive

Groups	N	Mean ± SD	Minimum	Maximum
Composite bur	30	3.60±1.19	1	5
Tungsten carbide bur	30	2.93±1.11	1	5
Er:YAG	30	3.79±1.93	1	9

ANOVA; $P = 0.069$; $P < 0.05$ indicates a significant result after analysis of variance; Values are presented as number and mean ± SD and minimum and maximum; SD: Standard deviation; Er:YAG: Erbium-doped yttrium aluminum garnet.

the cutting edges of tungsten carbide bur remove a significant amount of enamel.

Thermal changes of the pulp chamber in different groups were not similar. The temperature of the pulp chamber increased significantly in composite bur and tungsten carbide bur groups while decreased significantly in Er:YAG laser group. This decrease in temperature was apparently related to the cooling air and water system in Er:YAG laser application. These

results are consistent with earlier researches.^[17,18,20] There is a controversy over thermal effect of tungsten carbide bur. Mank *et al.*^[21] stated that in the absence of air or water cooling system, the temperature of the pulp chamber did not significantly increase while Ozer *et al.*^[26] suggested low speed hand piece with air cooling, and Uysal *et al.*^[4] showed a decrease in temperature by 5.36°C when cooling water was applied. These two later results are consistent with our result.

In the present study, it took 56.53 s for tungsten carbide bur and 37.85 s for composite bur to increase the temperature by 5.5°C. Since increased temperature by 5.5°C may lead to irreversible pulp tissue inflammation (in 40% of cases), it is suggested to apply air or water cooling system, or work intermittently when using tungsten carbide or composite burs.

The time consumed to remove adhesive residue from the enamel surface depends largely on the amount of remnant adhesive. In this study, the distribution of ARI scores for the experimental groups were broadly similar and the ARI score two was the most frequent score; hence, the groups were comparable. Although, no significant differences were observed between groups, tungsten carbide bur took shorter time than two other methods to remove adhesive residue. This might be related to having sharp cutting edges on this bur while composite bur works by means of abrasion. Er:YAG laser was the slowest.

CONCLUSION

1. SEM images showed that composite bur created the smoothest enamel surface while Er:YAG laser the roughest.
2. Tungsten carbide and composite burs generated significantly more heat compared to Er:YAG laser.
3. Temperature of the pulp chamber increased by 5.5°C in 56.36 and 37.86 s by tungsten carbide and composite burs, respectively.
4. Tungsten carbide bur was the fastest and Er:YAG laser the slowest devices to remove adhesive residue.

Regarding the results of the present study, composite bur with air or water cooling system, because of being less harmful to enamel and pulp tissue, is recommended to remove the residual adhesive following orthodontic bracket debonding.

ACKNOWLEDGMENTS

This study was supported by a grant number 2537 of Research Vice Chancellor of Shahid Sadoughi University of Medical Sciences.

REFERENCES

1. Ogaard B, Brantley WA, Eliades T, editors. Oral microbiological changes, long term enamel alterations due to decalcification and caries prophylactic aspects. Orthodontic Materials: Scientific and Clinical Aspects. Stuttgart, Germany: Thieme; 2001. p. 124-39.
2. Radlanski RJ. A new carbide finishing bur for bracket debonding. J Orofac Orthop 2001;62:296-304.
3. Banerjee A, Paolinelis G, Socker M, McDonald F, Watson TF. An *in vitro* investigation of the effectiveness of bioactive glass air-abrasion in the 'selective' removal of orthodontic resin adhesive. Eur J Oral Sci 2008;116:488-92.
4. Uysal T, Eldeniz AU, Usumez S, Usumez A. Thermal changes in the pulp chamber during different adhesive clean-up procedures. Angle Orthod 2005;75:220-5.
5. Kim SS, Park WK, Son WS, Ahn HS, Ro JH, Kim YD. Enamel surface evaluation after removal of orthodontic composite remnants by intraoral sandblasting: A 3-dimensional surface profilometry study. Am J Orthod Dentofacial Orthop 2007;132:71-6.
6. Cook RJ, Azzopardi A, Thompson ID, Watson TF. Real-time confocal imaging, during active air abrasion — Substrate cutting. J Microsc 2001;203:199-207.
7. Chan KH, Hirasuna K, Fried D. Rapid and selective removal of composite from tooth surfaces with a 9.3 μm CO2 laser using spectral feedback. Lasers Surg Med 2011;43:824-32.
8. Dumore T, Fried D. Selective ablation of orthodontic composite by using sub-microsecond IR laser pulses with optical feedback. Lasers Surg Med 2000;27:103-10.
9. Hibst R, Keller U. Removal of dental filling materials by Er:YAG laser radiation. In: Lasers in Orthopedic, Dental, and Veterinary Medicine. SPIE Proceedings 1991;1424:120-6.
10. Nelson JS, Yow L, Liaw LH, Macleay L, Zavar RB, Orenstein A, *et al.* Ablation of bone and methacrylate by a prototype mid-infrared erbium:YAG laser. Lasers Surg Med 1988;8:494-500.
11. Marshall S, Marshall G, Watanabe L, White J. Effects of the Nd:YAG laser on amalgams and composites. Trans Acad Dent Mater 1989;2:297-308.
12. Thomas BW, Hook CR, Draughn RA. Laser-aided degradation of composite resin. Angle Orthod 1996;66:281-6.
13. Yow L, Nelson JS, Berns MW. Ablation of bone and polymethylmethacrylate by an XeCl (308 nm) excimer laser. Lasers Surg Med 1989;9:141-7.
14. Sherk HH, Lane G, Rhodes A, Black J. Carbon dioxide laser removal of polymethylmethacrylate. Clin Orthop Relat Res 1995;310:67-71.
15. Karan S, Kircelli BH, Tasdelen B. Enamel surface roughness after debonding. Angle Orthod 2010;80:1081-8.
16. Almeida HC, Vedovello Filho M, Vedovello SA, Young AA, Ramirez-Yañez GO. ER: YAG laser for composite removal after bracket debonding: A qualitative SEM analysis. Int J Orthod Milwaukee 2009;20:9-13.

17. Burkes EJ Jr, Hoke J, Gomes E, Wolbarsht M. Wet versus dry enamel ablation by Er:YAG laser. *J Prosthet Dent* 1992;67:847-51.
18. Theodoro LH, Haypek P, Bachmann L, Garcia VG, Sampaio JE, Zezell DM, *et al.* Effect of ER:YAG and diode laser irradiation on the root surface: Morphological and thermal analysis. *J Periodontol* 2003;74:838-43.
19. Zach L, Cohen G. Pulp response to externally applied heat. *Oral Surg Oral Med Oral Pathol* 1965;19:515-30.
20. Park NS, Kim KS, Kim ME, Kim YS, Ahn SW. Changes in intrapulpal temperature after Er:YAG laser irradiation. *Photomed Laser Surg* 2007;25:229-32.
21. Mank S, Steineck M, Brauchli L. Influence of various polishing methods on pulp temperature: An *in vitro* study. *J Orofac Orthop* 2011;72:348-57.
22. David VA, Staley RN, Bigelow HF, Jakobsen JR. Remnant amount and cleanup for 3 adhesives after debracketing. *Am J Orthod Dentofacial Orthop* 2002;121:291-6.
23. Brauchli LM, Baumgartner EM, Ball J, Wichelhaus A. Roughness of enamel surfaces after different bonding and debonding procedures: An *in vitro* study. *J Orofac Orthop* 2011;72:61-7.
24. Al Shamsi AH, Cunningham JL, Lamey PJ, Lynch E. Three-dimensional measurement of residual adhesive and enamel loss on teeth after debonding of orthodontic brackets: An *in-vitro* study. *Am J Orthod Dentofacial Orthop* 2007;131:301.e9-15.
25. Eliades T, Gioka C, Eliades G, Makou M. Enamel surface roughness following debonding using two resin grinding methods. *Eur J Orthod* 2004;26:333-8.
26. Ozer T, Başaran G, Kama JD. Surface roughness of the restored enamel after orthodontic treatment. *Am J Orthod Dentofacial Orthop* 2010;137:368-74.
27. Artun J, Bergland S. Clinical trials with crystal growth conditioning as an alternative to acid-etch enamel pretreatment. *Am J Orthod* 1984;85:333-40.
28. Howell S, Weekes WT. An electron microscopic evaluation of the enamel surface subsequent to various debonding procedures. *Aust Dent J* 1990;35:245-52.

How to cite this article: Yassaei S, Aghili H, Joshan N. Effects of removing adhesive from tooth surfaces by Er:YAG laser and a composite bur on enamel surface roughness and pulp chamber temperature. *Dent Res J* 2015;12:254-9.

Source of Support: This research was funded by Shahid Sadoughi University of Medical Sciences. **Conflict of Interest:** The authors of this manuscript declare that they have no conflicts of interest, real or perceived, financial or non-financial in this article.